



IEC 60695-11-3:2012 specifies the apparatus, operating conditions and confirmational test methods required to produce standardized **500 W nominal premixed test flames** for fire-hazard آزمون.

Unlike IEC 60695-11-4, which specifies a 50 W flame, IEC 60695-11-3 addresses a substantially higher-energy **500 W flame**, with an approximate overall flame height of **125 mm**.

The standard defines two valid methods

- **Method A** – 500 W premixed methane flame using adjustable, existing-type burner hardware
- **Method C** – 500 W premixed methane or propane flame using specially developed non-adjustable burner hardware

Methods B and D, which appeared in earlier technical specifications, have been withdrawn.

Both current methods are designed to produce a standardized flame with comparable thermal performance, which is verified by heating a specified copper block from **100 °C to 700 °C in 54 ± 2 seconds**.

:This article provides a detailed technical overview of

- operating principle
- Method A
- Method C
- burner construction
- burner dimensions
- fuel requirements
- gas and air flow requirements
- back-pressure requirements
- flowmeters and manometers
- copper calibration block
- thermocouple
- دما and time اندازه گیری
- آزمایشگاه chamber
- flame geometry
- flame-height gauge
- flame production

- ;calibration and confirmation
- ;acceptance criteria
- ;equipment test arrangements
- ماده ;test arrangements
- and the principal differences between Method A and Method C.

1. دامنه کاربرد IEC 60695-11-3

IEC 60695-11-3 specifies detailed requirements for producing either of two standardized

W nominal premixed test flames 500

The approximate overall height of either flame is: **125 mm**

The two methods differ primarily in burner construction and control of the fuel/air mixture.

Method A

Method A uses: **Methane only** and is based on adjustable existing-type burner hardware.

Method C

Method C uses either: **Methane** or: **Propane**

and employs specially developed **non-adjustable burner hardware** with separately controlled fuel and air supplies. Despite the different methods of producing the flame, both methods use the same basic thermal confirmation principle.

Standardized 500 W Test Flame .2

:A flame should not be considered a standardized IEC 60695-11-3 flame merely because

- ;it visually appears similar
- ;it has an approximately 125 mm height
- or the burner is rated nominally at 500 W.

Compliance depends on the complete system.

:The specified

- ;burner geometry
- ;fuel

- ;fuel purity
- ;fuel flow
- ;air supply where applicable
- فشار conditions
- ;flame dimensions
- ;chamber conditions
- ;copper block
- ;thermocouple
- اندازه گیری system
- and thermal confirmation result

must all be considered. The ultimate confirmation is based on the thermal response of a standardized copper block.

3. Flame Geometry

Both Method A and Method C produce approximately the same specified flame geometry.

Overall Flame Height Approximately 125 mm

Inner Blue Cone Height Approximately 40 mm

The standard's Figure 1 defines these two primary flame dimensions.

:During calibration, the flame shall also be

- ;stable
- ;symmetrical
- ;correctly premixed
- and capable of satisfying the specified copper-block heating test.

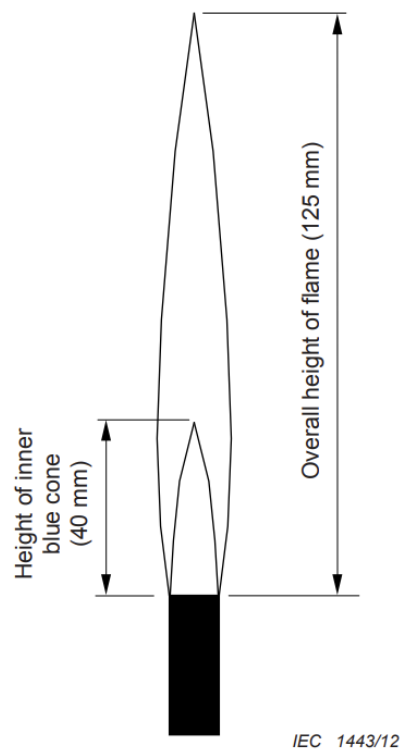


Figure 1 – Flame dimensions

Overview of Method A .4

Method A is based on existing adjustable burner hardware.

The burner uses: **Methane ≥ 98 % purity** with a specified gas flow and back فشار.

The burner includes an adjustable air inlet, which is used to establish the required inner blue cone.

The principal operating values are: Methane Flow **965 ± 30 ml/min** corrected to: **23 °C and 0.1 MPa**

Gas Back فشار 5 mm water column ± 125

Inner Blue Cone approximately 40 mm

Overall Flame Height approximately 125 mm

Confirmational Heating Time 54 ± 2 s

for the copper block to increase from: **100 ± 2 °C to 700 ± 3 °C**

Method A - Burner Construction .5

:The Method A burner consists essentially of

- ;burner tube
- ;valve seat / gas injector
- ;lock nut
- ;main body
- ;needle valve
- ;needle-valve packing
- ;needle-valve packing nut
- ;adjustable needle-valve stop
- adjustable air inlet.

The burner tube, gas injector and needle valve can be removed for cleaning. During reassembly, particular care must be taken to avoid

- ;damage to the needle-valve tip
- ;misalignment of the needle valve
- misalignment between the needle valve and valve seat.

These conditions can affect gas regulation and consequently alter flame geometry and thermal output.

Method A - Burner Tube Dimensions .6

:The detailed Method A burner drawing specifies

Burner Tube Internal Diameter $\varnothing 9.5 \pm 0.3$ mm

Burner Tube Length 100 ± 10 mm

Lower Internal Diameter $\varnothing 18$ mm

Air Inlet Three slots are: equally spaced around the burner diameter

The minimum total air-inlet area is: **225 mm²**

The adjustable air inlet enables the operator to control the premixed air/fuel condition and consequently the inner blue cone height.

Method A - Gas Injector .7

The specified gas orifice diameter is: $\varnothing 0.9 \pm 0.03 \text{ mm}$

:The detailed valve-seat geometry also specifies

- a 40° feature
- $\varnothing 10 \pm 0.2 \text{ mm} \times 2 \text{ mm}$ deep geometry
- other specified machining dimensions
- maximum flat at the top of the needle/seal region: **0.4 mm**

The exact geometry is important because gas velocity and mixing behaviour are directly influenced by the injector.

Method A - Burner .8 and General Tolerances

ﻻﺩﻩ The burner is manufactured from: **brass or another suitable**

:Unless otherwise stated, Method A burner drawing tolerances are

For dimensions shown as whole numbers: **$\pm 0.5 \text{ mm}$**

For dimensions shown to one decimal place: ± 0.1 mm

For angular dimensions: ± 30 minutes

unless a specific tolerance is separately given.

Method A - Gas Supply Arrangement .9


:The typical gas supply arrangement consists of

Fuel Gas Source → Control Valve → Gas Flowmeter → Manometer → Burner

:The burner then provides

- needle-valve adjustment
- adjustable air inlet.

drop. All gas فشار The tubing between the flowmeter and burner shall have sufficient internal diameter to minimize connections shall be leak-free.

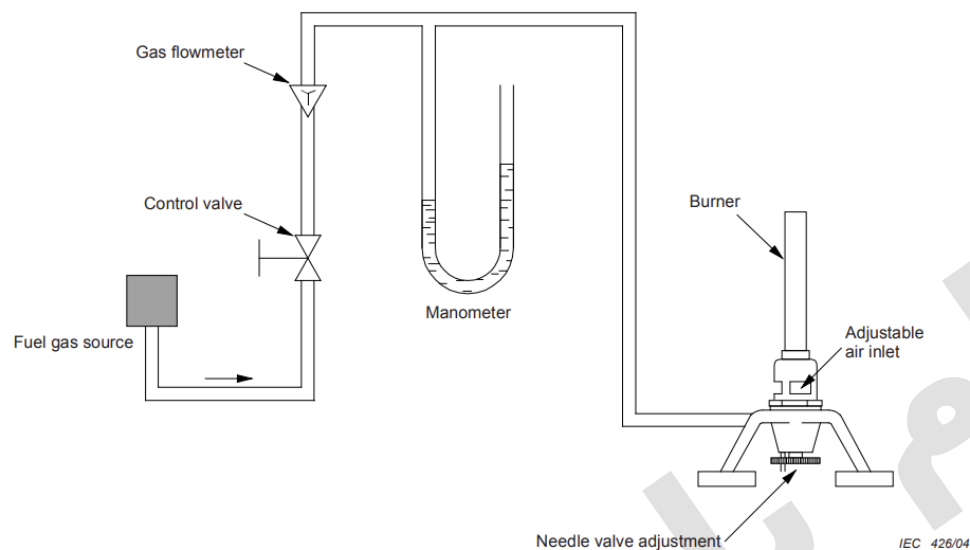

NOTE 1 A manometer is required in conjunction with a mass flowmeter in order to maintain the required back pressure.

NOTE 2 The inner diameter of the tubes connecting the flowmeters to the burner must be of adequate size to minimize pressure drop.

Figure A.2 – Supply arrangement for burner (example)

10. Method A - Methane الزامات

% Method A uses: **Methane** with minimum purity: **98**

Required gas flow: **965 ± 30 ml/min** at the reference conditions: **23 °C and 0.1 MPa**

Where اندازه گیری are made under actual آزمایشگاه. conditions, they must be corrected to the specified reference conditions.

11. Method A - Flowmeter

The gas flowmeter shall be appropriate for measuring: **965 ml/min methane**

% at: **23 °C and 0.1 MPa** with a tolerance of: **±2**

A mass flowmeter is the preferred method for accurately controlling the fuel input.

Alternative methods may be used where equivalent accuracy can be demonstrated.

Method A - Manometer .12

The manometer shall be suitable for measuring: **0 to 7.5 kPa**

A water manometer may be used when adapted to cover this range.

For Method A, فشار اندازه گیری burner back is particularly important because the specified gas condition includes a burner back **125 ± 5 mm water column** of: فشار

When a mass flowmeter is used, a manometer is still required to maintain the required back فشار.

Method A - Control Valve .13

A control valve is required to establish the gas flow.

The complete adjustment of Method A therefore involves interaction between

- external gas-flow control
- gas back فشار;
- burner needle valve

• and adjustable air inlet.

The final flame is accepted based on both geometry and thermal confirmation.

14. Method A - Flame Production

The burner supply system is assembled according to the specified Method A arrangement.

chamber. The methane آزمایشگاه All connections shall be checked to ensure they are leak-free. The burner is installed in the is ignited.

are adjusted to: **965 ± 30 ml/min** and: **125 ± 5 mm H₂O** respectively. فشار Gas flow and back

The air inlet is then adjusted until the inner blue cone is approximately: **40 mm**

The air inlet is locked in position using the lock nut.

The resulting flame shall appear: **stable and symmetrical**

Method A - Calibration Flame Dimensions .15

During the confirmational procedure, the inner blue cone is adjusted more precisely to: **40 ± 2 mm** using the specified flame-height gauge.

the operator, اندازه گیری, The overall flame height shall be approximately: **125 mm** The air inlet is then locked. Before thermal verifies

- gas flow ;
- gas back فشار ;
- blue-cone height ;
- flame symmetry.

Method C - Operating Principle .16

Method C takes a different engineering approach. Rather than relying on adjustable burner hardware to entrain and regulate air, it uses: **non-adjustable burner hardware**

:with independent supplies for


- fuel gas ;

• compressed air.

The burner was specifically developed to provide a highly repeatable and stable 500 W flame.

Method C can operate using: **methane**

.or: **propane**

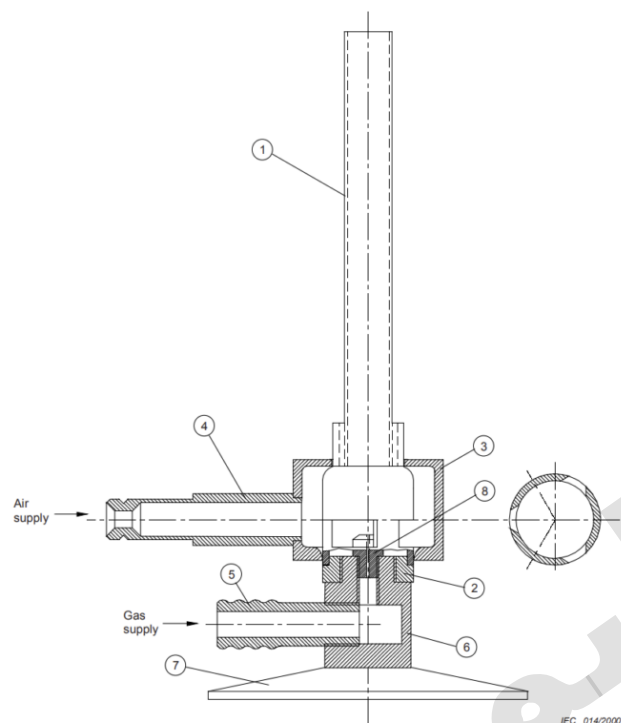


Key

- 1 burner barrel
- 2 O rings
- 3 air manifold
- 4 air supply tube
- 5 gas supply tube
- 6 elbow block
- 7 burner base
- 8 gas jet

Parts 1, 2, 3 and 4 are hard-soldered on assembly.
Parts 5 and 6 may be hard-soldered together, if necessary, to prevent leakage of gas.
Parts 7 and 8 may be fabricated in one piece, or fastened together, to prevent gas leakage.
Parts 1, 2, 3 and 4 are detailed in Figure B.2.
Parts 5 and 8 are detailed in Figure B.3.
Parts 6 and 7 are detailed in Figure B.4.

Figure B.1 – Burner, method C – General assembly

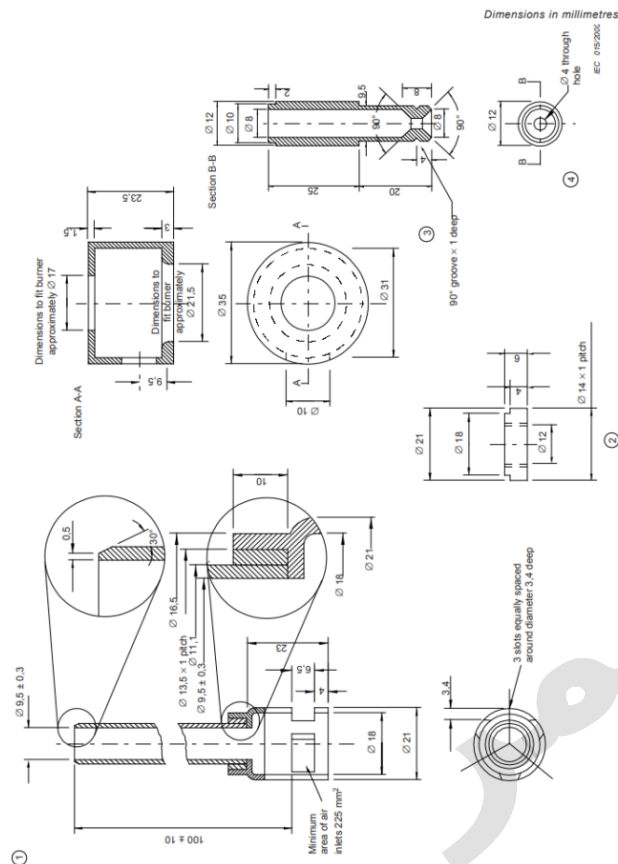

Material: brass or any other suitable material

Tolerances on linear dimensions: ± 0.1 mm, unless otherwise stated.

Tolerances on angular dimensions: ± 30 min, unless otherwise stated.

Figure B.2 – Burner details – Burner barrel, O-ring, air manifold and air supply tube

Method C - Burner Assembly .17


:The Method C burner consists of eight principal components

1. Burner barrel
2. O-rings
3. Air manifold
4. Air supply tube
5. Gas supply tube
6. Elbow block
7. Burner base
8. Gas jet

The assembly is specifically designed to control mixing without an adjustable burner air inlet. Parts 1, 2, 3 and 4 are hard-soldered during assembly.

:Parts 5 and 6 may be hard-soldered together where necessary to prevent gas leakage. Parts 7 and 8 may either

- ;be fabricated as a single piece
- or be securely joined to prevent gas leakage.

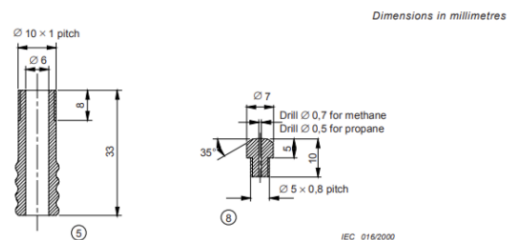


Material: brass or any other suitable material

Tolerances on linear dimensions: $\pm 0,1$ mm, unless otherwise stated.

Tolerances on angular dimensions: ± 30 min, unless otherwise stated.

Figure B.3 – Burner details – Gas supply tube and gas jet

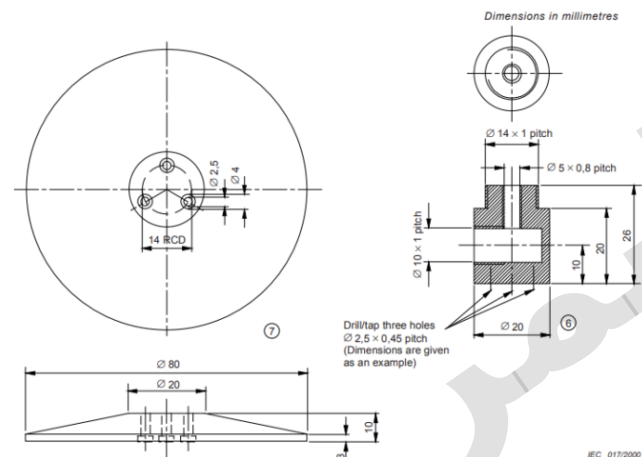

Material: brass or any other suitable material

Tolerances on linear dimensions: $\pm 0,1$ mm, unless otherwise stated.

NOTE The shape of part 7 is given as an example.

Figure B.4 – Burner details – Burner base and elbow block

Method C - Burner Barrel .18

The burner barrel has the principal dimensions: Internal Diameter $\varnothing 9.5 \pm 0.3 \text{ mm}$ Length $100 \pm 10 \text{ mm}$

The air manifold provides air through: **3 slots equally spaced around the diameter**
with a minimum total air-inlet area of: **225 mm²**

The detailed construction also includes the O-ring, air manifold and air supply tube geometry specified in the standard.

Method C - Burner .19 and Tolerances

ماده The Method C burner components are specified as: **brass or another suitable**

For the detailed burner components, unless otherwise specified: Linear Tolerance $\pm 0.1 \text{ mm}$ Angular Tolerance ± 30
minutes

This is an important distinction from some of the general dimensional tolerances shown for the Method A burner.

Method C - Gas Jet .20

Method C uses different gas-jet drilling depending on fuel.


Methane Jet Ø 0.7 mm

Propane Jet Ø 0.5 mm

:The jet drawing also specifies

- geometry 35°
- ;Ø5 × 0.8 pitch thread
- ;Ø10 × 1 pitch features
- associated length and machining dimensions.

Correct selection of the jet is essential because methane and propane require different volumetric flow rates.

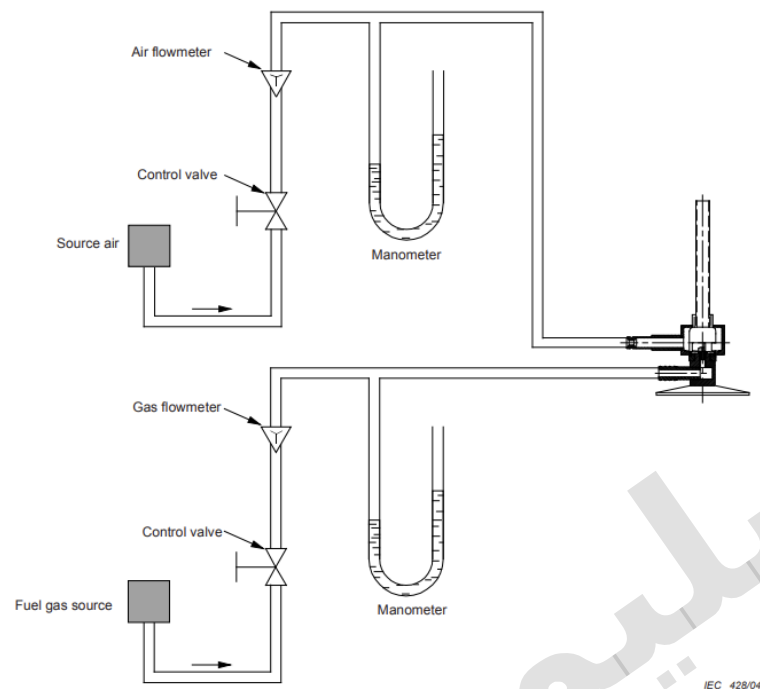

The inner diameter of the tubes connecting the flowmeters to the burner must be of adequate size to minimize pressure drop.

Compressed air to be essentially free of oil and water.

NOTE Manometers are not required when mass flowmeters are used.

Figure B.5 – Supply arrangement for burner (example)

Method C - Methane Operating Conditions .21

:When Method C is operated with methane

% Methane Purity ≥ 98

Methane Flow 965 ± 30 ml/min at: 23°C and 0.1 MPa

Air Flow 6.3 ± 0.1 l/min at: 23°C and 0.1 MPa

Expected Methane Back فشار 110-170 mm water

Expected Air Back فشار 20-40 mm water

These فشار ranges are expected operating values rather than the principal flow-setting criteria.

Method C - Propane Operating Conditions .22

:When Method C is operated with propane

% Propane Purity ≥ 98

Propane Flow 380 ± 15 ml/min at: 23°C and 0.1 MPa

Air Flow 5.9 ± 0.1 l/min at: 23°C and 0.1 MPa

205 mm water-135 فشار Expected Propane Back

35 mm water-15 فشار Expected Air Back

Methane Requirement in Case of Dispute .23

:Although Method C permits either methane or propane during normal use, IEC 60695-11-3 specifies that

in cases of dispute, methane shall be used

% with a purity of at least: 98

This is an important requirement when results from different laboratories or parties need to be formally compared.

Method C - Air Supply Quality .24

:The compressed air supplied to the Method C burner shall be essentially free from

- oil ;
- water.

Contamination of the air supply can affect burner operation, mixture characteristics and repeatability.

Method C - Flowmeters .25

Separate اندازه گیری for is required :

- fuel flow ;
- air flow.

Fuel flowmeters shall measure: Methane **965 ml/min** or: Propane **380 ml/min** at the specified reference conditions.

Air flowmeters shall measure: Methane configuration **6.3 l/min** or: Propane configuration **5.9 l/min**

Required flow اندازه گیری $\pm 2\%$ tolerance:

Mass flowmeters are preferred for accurate control of both fuel and air.

Method C - Manometers .26

Where conventional flow اندازه گیری is used, two manometers are required

- one for fuel
- one for air.

Each shall be suitable for: **0-7.5 kPa**

:Water manometers may be used. However, unlike Method A

manometers are not required when mass flowmeters are used for Method C.

Method C - Control Valves .27

Two control valves are required: Gas Control Valve for fuel-flow adjustment. Air Control Valve for air-flow adjustment. This permits independent establishment of the specified gas and air flow rates.

Method C - Supply Arrangement .28

The Method C supply arrangement contains two separate circuits.

Air Circuit

Burner → فشار اندازه گیری → Air Source → Control Valve → Air Flowmeter

Fuel Circuit

Burner → فشار اندازه گیری → Fuel Source → Control Valve → Gas Flowmeter

drop. The compressed air shall remain فشار The internal diameter of connecting tubes shall be sufficient to minimize

essentially free from oil and water.

Method C - Flame Production .29

Assemble the burner supply arrangement and verify that all gas and air connections are leak-free. Place the burner inside chamber. آزمایشگاه the

Ignite the mixture.

:Adjust the gas and air flow rates to the appropriate values for either

- ;methane operation
- or propane operation.

The resulting flame shall have: **Inner blue cone $\approx$ 40 mm Overall flame height $\approx$ 125 mm** and shall appear: **stable and symmetrical**

Copper Confirmation Block .30

Both Method A and Method C use the same standardized copper block for thermal confirmation.

High-conductivity electrolytic copper: Cu-ETP / UNS C11000 ماده

Diameter $\varnothing 9 \pm 0.01$ mm

Mass Before Drilling 10.00 ± 0.05 g

Thermocouple Hole $\varnothing 0.5$ mm

Principal Drawing Dimensions

0.02 mm ± 19.14

0.04 mm ± 20.64

0.02 mm ± 6


Lower Angles $45^\circ \pm 0.5^\circ$

The block shall be: **polished all over**

Unless otherwise specified: Linear Tolerance ± 0.1 mm

Angular Tolerance ± 30 min

آوا هونام پلیمر

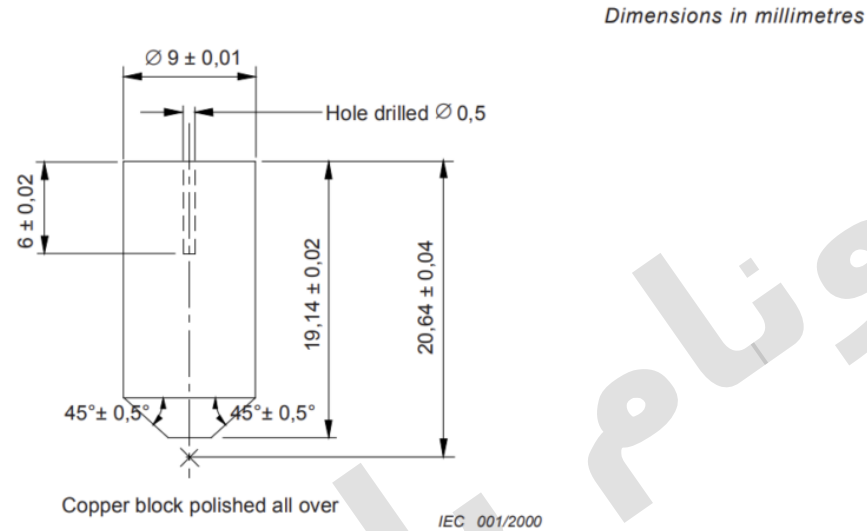


Tolerances on linear dimensions: $\pm 0,1$ mm, unless otherwise stated.

Tolerances on angular dimensions: ± 30 min, unless otherwise stated.

Material: high conductivity electrolytic copper Cu-ETP UNS C 11000 (see ASTM-B187/B187M-06)

Mass: $10 \text{ g} \pm 0,05 \text{ g}$ before drilling.

Figure 2 – Copper block

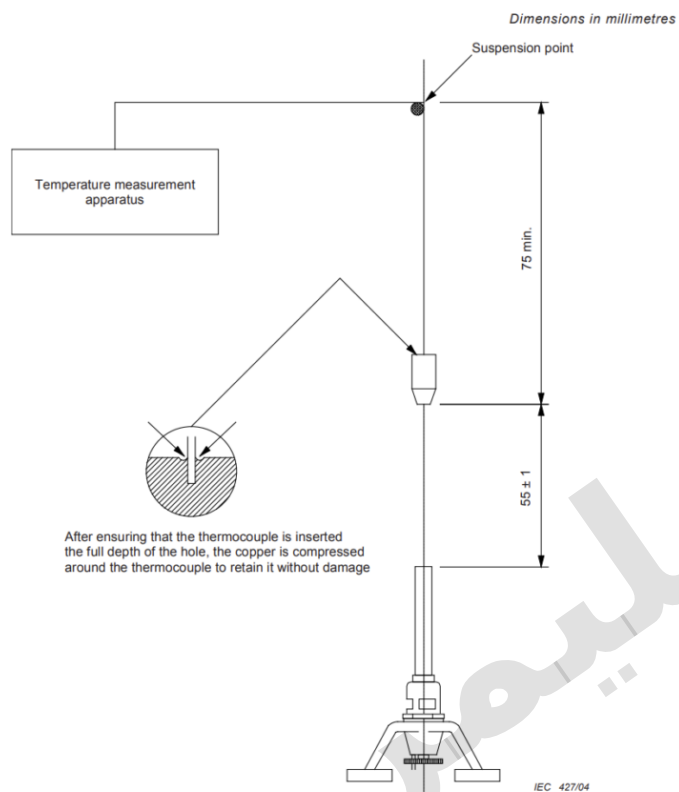

The mode of suspension of the copper block shall be such that the copper block remains essentially stationary during the test.

Figure A.3 – Confirmatory test arrangement

31. Copper Block Reference Control

IEC 60695-11-3 does not define a separate verification procedure for the copper block itself.

Laboratories are encouraged to maintain

- a standard reference unit
- a secondary standard reference unit
- a working unit.

Cross-comparison can then be used to verify the working system.

This is important because variations in

- copper mass
- geometry
- ماده
- machining
- surface condition
- thermocouple installation

can influence heating time.

32. Thermocouple الزامات

Both methods use a: **mineral-insulated, metal-sheathed fine-wire thermocouple**
with: **insulated junction**

The thermocouple shall be: **IEC 60584-2 Class 1**

Nominal overall diameter: **0.5 mm**

An example is: **Type K - NiCr/NiAl**

according to IEC 60584-1. The welded point is located inside the sheath.

33. Capability دما Thermocouple

The thermocouple sheath shall consist of a metal capable of continuous operation at: **at least 1,050 °C** capability is necessary even though دما A suitable nickel-based heat-resistant alloy can satisfy this requirement. This high-ends at 700 °C. اندازه گیری the confirmational

34. Thermocouple Installation in the Copper Block

The thermocouple shall first be inserted to: **the full depth of the drilled hole**
The preferred retention method is then to: **compress the copper around the thermocouple**
so that it is securely retained without damaging the sensor. This arrangement is shown in both Method A and Method C confirmational test diagrams.

35. دما and Time اندازه گیری

The دما time indicating or recording system shall be capable of determining the time required for the copper block to rise/دما from: **100 ± 2 °C** to: **700 ± 3 °C**

The tolerance on measured time shall be: **±0.5 s**

The recording system therefore needs sufficient

- دما accuracy
- response
- sampling performance
- time resolution

to determine this heating interval reliably.

36. آزمایشگاه Fumehood / Chamber

Both methods require a chamber with an internal volume of at least: **0.75 m³** آزمایشگاه

:The chamber shall

- ;permit observation of the test
- ;provide a draught-free environment
- allow normal thermal circulation of air around the sample; نمونه آزمون;
- have dark-coloured internal walls.

The chamber is an integral part of the test system because airflow can substantially affect a 125 mm premixed flame.

37. Chamber Illumination

A lux meter is positioned at the flame location and directed toward the rear of the chamber.

The measured background illumination shall be: **<20 lx**

This provides appropriate conditions for visual evaluation of the flame.

38. Chamber Extraction System

The enclosure may be equipped with an extraction device such as an exhaust fan to remove combustion products.

However: **Extraction shall be OFF during the test.**

Immediately after the test: **Extraction shall be switched ON**

to remove potentially toxic fire effluents.

A positive-closing damper may be required.

39. Chamber Oxygen Availability

The standard specifically notes that oxygen availability is important during flame **آزمون.**

For tests involving prolonged burning: **a 0.75 m³ chamber may not necessarily be sufficient**

to produce accurate results.

Therefore, chamber volume should not be interpreted independently from the combustion duration and oxygen demand of

the actual test.

40. Flame Height Gauge

The flame-height gauge is used to establish the required

- 40 mm inner blue cone
- 125 mm overall flame height.

The gauge is manufactured from: **1.0 to 1.5 mm steel plate**


and incorporates thermally insulating strips.

Principal dimensions include

- overall reference height: **135 ± 0.5 mm**
- gauge width: **30 mm**
- reach: **120 mm**
- reference sections including **20 ± 0.5 mm**, **38 ± 0.5 mm**, and **4 ± 0.5 mm**
- specified 20° and 30° reference angles.

Unless otherwise stated, gauge tolerances are: Linear $\pm 1 \text{ mm}$ Angular $\pm 5^\circ$

آوا هونام پلیمر

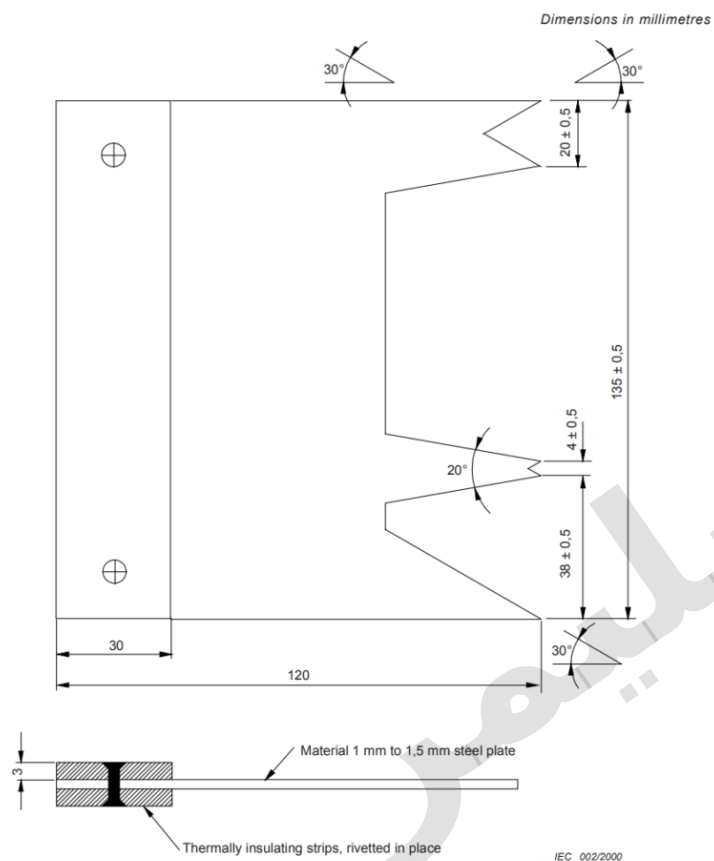

Tolerances on linear dimensions: ± 1 mm, unless otherwise stated.

Tolerances on angular dimensions: $\pm 5^\circ$, unless otherwise stated.

Figure 3 – Flame height gauge

41. Principle of Thermal Confirmation

The flame is not finally accepted by visual inspection.

The standard uses a quantitative thermal test.

The standardized copper block is suspended above the burner.

The burner is positioned according to the relevant confirmational arrangement.

The system records the time required for the copper block to increase from: $100 \pm 2 \text{ }^{\circ}\text{C}$ to: $700 \pm 3 \text{ }^{\circ}\text{C}$ اندازه گیری

The required result for both methods is: **$54 \pm 2 \text{ seconds}$**

Therefore, each acceptable determination must fall within: **52-56 seconds**

42. Confirmational Test Geometry

For both Method A and Method C, the copper block shall be suspended so that it remains essentially stationary during the :test. The confirmational drawings specify

Minimum Suspension Dimension 75 mm minimum

Burner-to-Block Reference Dimension 55 ± 1 mm

The burner is positioned directly below the copper block according to the specified geometry.

Method A uses the arrangement shown for its adjustable burner.

Method C uses the corresponding arrangement for the non-adjustable burner.

43. Method A - Complete Confirmation روش اجرا

Step 1 - Assemble the System

Set up the burner supply and confirmation arrangement. Place it inside the specified chamber. Ensure that all gas connections are leak-free.

Step 2 - Move Burner Away from Copper Block

Temporarily remove the burner from beneath the copper block. This prevents preliminary flame adjustment from influencing the block.

Step 3 - Ignite Methane

Ignite the gas.

Step 4 - Adjust Gas Flow

Set methane flow to: **965 ± 30 ml/min** at the specified reference conditions.

Step 5 - Adjust Back فشار

Set: **125 ± 5 mm H₂O**

Step 6 - Adjust Inner Blue Cone

Adjust the burner air inlet until the blue cone is: **40 ± 2 mm**

Step 7 - Lock Air Adjustment

Secure the air inlet using the lock nut.

Step 8 - Verify Overall Flame

Confirm: **overall flame height ≈ 125 mm**

and ensure that the flame is symmetrical.

Step 9 - Stabilize Burner

Allow the burner to operate for at least: **5 minutes** to reach equilibrium.

Step 10 - Recheck Parameters

:Confirm that

- gas flow
- gas back فشار;
- blue-cone height

remain within the prescribed limits.

Step 11 - Begin Thermal Test

Ensure that the system is operating. time/دما اندازه گیری.


Move the burner back underneath the copper block.

Step 12 - Measure Heating Time

Measure the time required for: $100 \pm 2 \text{ }^{\circ}\text{C} \rightarrow 700 \pm 3 \text{ }^{\circ}\text{C}$

Required: $54 \pm 2 \text{ s}$

Test arrangements – Method A

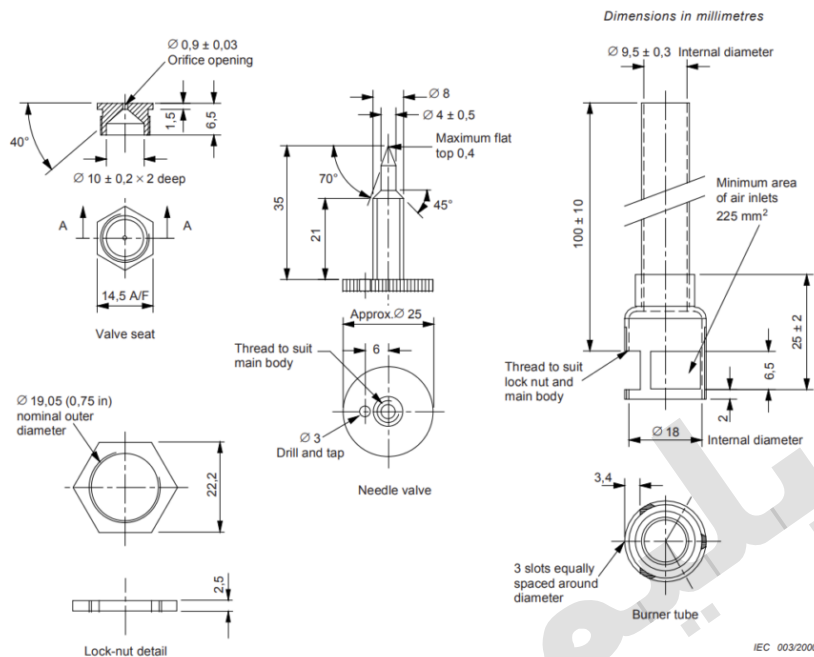

Material: brass or any other suitable material

Tolerances on linear dimensions:
xx (e.g. 20) means $\pm 0,5$ mm
xx.x (e.g. 20,0) means $\pm 0,1$ mm
unless otherwise stated.

Tolerances on angular dimensions:
x (e.g. 45) means ± 30 min
unless otherwise stated.

Figure A.1 (continued overleaf)

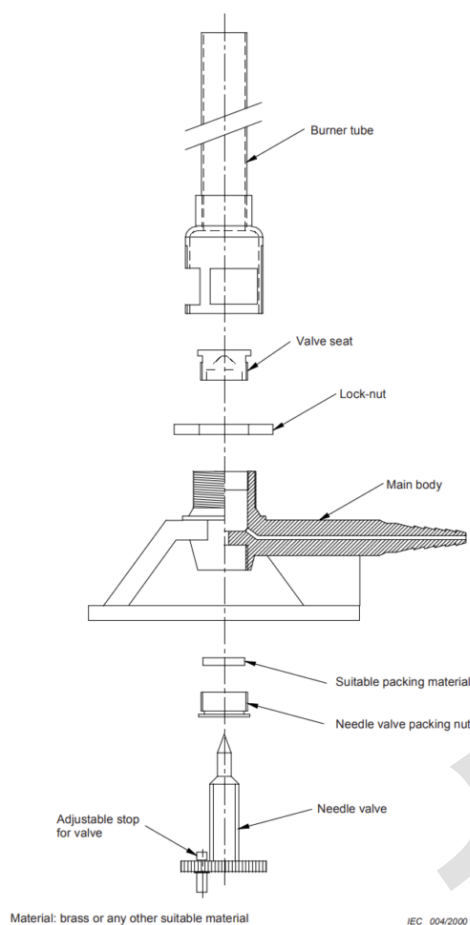


Figure A.1 – General assembly and details

44. Method C - Complete Confirmation روش اجرا

Step 1 - Assemble Burner and Supply System

Set up the Method C burner according to the specified confirmation arrangement.

:Ensure

- gas connections are leak-free
- air connections are leak-free.

Step 2 - Move Burner Away

Keep the flame away from the copper block during preliminary adjustment.

Step 3 - Ignite the Mixture

Ignite the selected fuel/air mixture.

Step 4 - Establish Flow Rates

For methane: **Gas = 965 ± 30 ml/min Air = 6.3 ± 0.1 l/min**

For propane: **Gas = 380 ± 15 ml/min Air = 5.9 ± 0.1 l/min**

Step 5 - Verify Flame Dimensions

:Using the flame-height gauge, verify

inner blue cone ≈ 40 mm

overall flame ≈ 125 mm

and ensure flame symmetry.

Step 6 - Stabilization

Wait at least: **5 minutes**

for burner equilibrium.

Step 7 - Recheck Flow Rates

Measure the fuel and air flows again and verify that they remain within the specified limits.


Step 8 - Position Burner

time recorder operating, move the burner beneath the copper block. / دما With the

Step 9 - Record Heating Time

Measure: $100 \pm 2 \text{ }^{\circ}\text{C} \rightarrow 700 \pm 3 \text{ }^{\circ}\text{C}$

Required result: $54 \pm 2 \text{ s}$

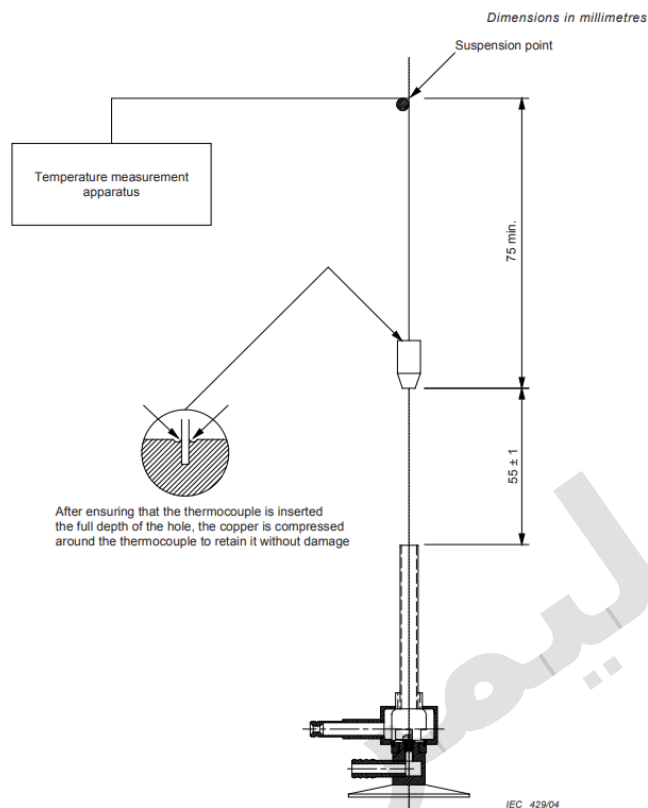

The mode of suspension of the copper block shall be such that the copper block remains essentially stationary during the test.

Figure B.6 – Confirmatory test arrangement

45. Three Successive Results Are Mandatory

For both methods, one compliant result is not sufficient.

After obtaining an acceptable result: **repeat the procedure twice**

until: **three successive determinations**

are within: **54 ± 2 s**

:Therefore

$52 \text{ s} \leq \text{Test 1} \leq 56 \text{ s}$

$52 \text{ s} \leq \text{Test 2} \leq 56 \text{ s}$

$52 \text{ s} \leq \text{Test 3} \leq 56 \text{ s}$

and the results must be consecutive.

46. Cooling Between Confirmational Tests

Between determinations, allow the copper block to cool: **naturally in air**

is: **below 50 °C** دما until its

Only then should another determination be performed.

47. Failed Confirmation Result

If any determination is outside: **54 ± 2 s**

the flame shall be adjusted accordingly.

:After adjustment

- allow the burner to return to equilibrium
- restart the confirmation procedure.

The requirement is not an average of several اندازه گیری s.

It is: **three successive compliant determinations.**

48. Conditioning a New Copper Block

:When a copper block is used for the first time

perform one preliminary heating cycle.

This conditions the block surface.

:The result shall be

discarded

and shall not count as one of the three confirmational اندازه گیری s.

49. Protection of the Thermocouple

The thermocouple may be easily damaged at temperatures above: **700 °C**.
It is therefore advisable to remove the burner immediately after the block reaches 700 °C.

50. Final Acceptance Criterion

For either Method A or Method C, the flame is confirmed and may be used for only when آزمون:

Range **100 ± 2 °C → 700 ± 3 °C**

Heating Time **54 ± 2 s**

Number of Required Results

3 successive compliant determinations

Cooling Between Runs Natural cooling to <50 °C

At least 5 minutes Burner Stabilization Before اندازه گیری

This thermal confirmation provides the practical verification that the complete burner system is producing the required standardized 500 W flame.

51. Designation دستگاه Classification and

:An apparatus satisfying Method A may be identified as

"W nominal test flame apparatus - Method A, conforming to IEC 60695-11-3. 500"

:An apparatus satisfying Method C may be identified as

"W nominal test flame apparatus - Method C, conforming to IEC 60695-11-3. 500"

52. Method A vs Method C - Technical Comparison

Parameter	Method A	Method C - Methane	Method C - Propane
-----------	----------	--------------------	--------------------

Nominal flame	W 500	W 500	W 500
Flame type	Premixed	Premixed	Premixed
Burner	Adjustable	Non-adjustable	Non-adjustable
Fuel	Methane	Methane	Propane
Fuel purity	% 98≤	% 98≤	% 98≤
Fuel flow	30 ml/min ± 965	30 ml/min ± 965	15 ml/min ± 380
Air supply	Burner air inlet	l/min 0.1 ± 6.3	l/min 0.1 ± 5.9
Fuel back فشار	5 mm H ₂ O ± 125	Expected 110-170 mm H ₂ O	Expected 135-205 mm H ₂ O
Air back فشار	—	Expected 20-40 mm H ₂ O	Expected 15-35 mm H ₂ O
Inner blue cone	40 mm	40 mm	40 mm
Overall flame	125 mm	125 mm	125 mm
Copper block	0.05 g ± 10.00	Same	Same
Confirmation	2 s ± 54	2 s ± 54	2 s ± 54

53. Recommended Arrangement for تجهیزات آزمون

equipment, unless the relevant product specification states otherwise, the recommended distance from: **the top of the burner tube** When either standardized 500 W flame is used for آزمون

surface نمونه آزمون to: the test point on the
is approximately: **55 mm**

The burner is fixed in position during the test.

The 55 mm distance was selected to improve reproducibility compared with trying to position the inner blue cone tip immediately adjacent to the نمونه آزمون.

Why the 55 mm Distance Is Used .54

distance provides better reproducibility than attempting to position نمونه آزمون The standard notes that the 55 mm burner-to-
the flame so that: **the tip of the inner blue cone just does not touch the** نمونه آزمون

which corresponds approximately to a separation of: **0-3 mm**

the fixed 55 mm burner reference is therefore, For equipment, نمونه آزمون. between the inner cone tip and recommended.

55. Bar نمونه آزمون

For bar-shaped نمونه آزمون, the test arrangement is different.
The operator may move the burner to follow a نمونه آزمون that:

- burns;
- bends;
- distorts.

In this case

the tip of the inner blue cone should just not touch the نمونه آزمون

corresponding to approximately: **0-3 mm clearance**

The burner is tilted so that falling debris does not enter the burner.

56. تجهیزات Test Orientation

The informative equipment test diagrams illustrate multiple application configurations.

:Examples include flame application to

- ;curved surfaces
- ;vertical surfaces
- edges or lower surfaces.

The illustrated arrangements use a burner inclination of approximately: **20°**

with the indicated: **55 mm**

reference distance. The relevant product specification ultimately determines the actual application geometry.

57. ماده Test Arrangements

:The standard also provides examples for

- sheet نمونه آزمون;

• strip نمونه آزمون.S.

ماده The informative drawings show possible burner orientations for applying the standardized 500 W flame to these configurations.

An inclination of approximately: **20°**

is illustrated for some arrangements.

ماده Again, these figures provide recommended arrangements; the applicable conditions and acceptance criteria.

Test arrangements for tests on equipment

Figure D.1 gives examples of test arrangements.

Dimensions in millimetres

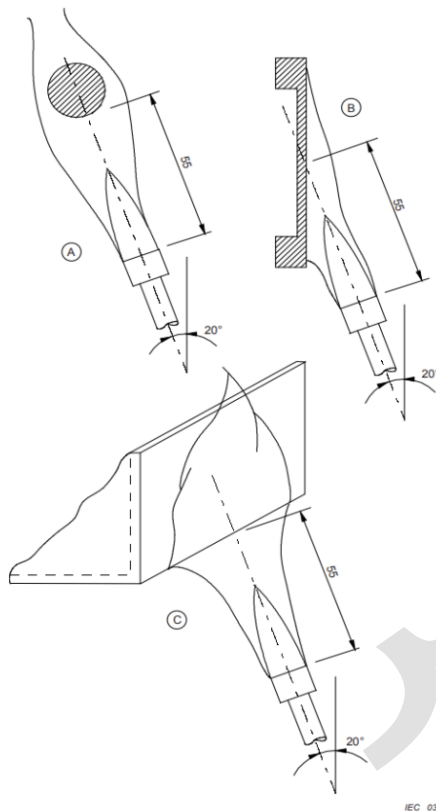


Figure D.1 – Examples of test arrangements

Test arrangements for tests on material

Figure E.1 gives examples of test arrangements.

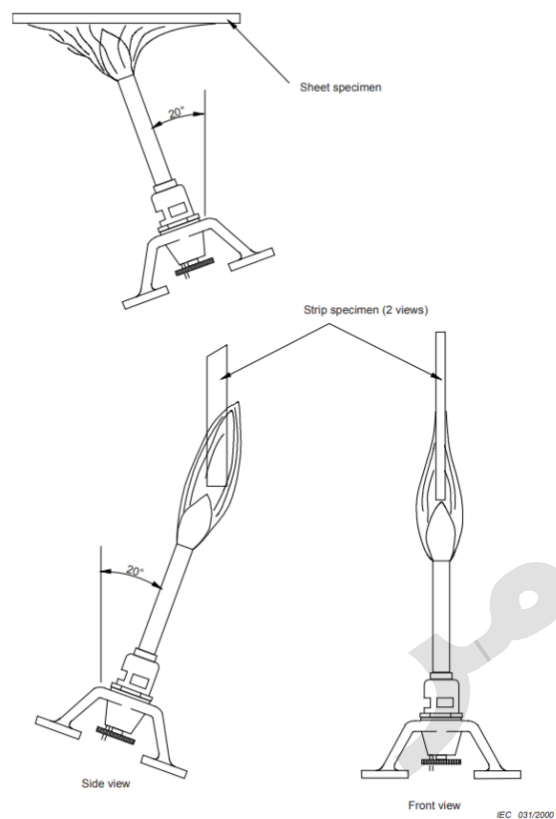


Figure E.1 – Examples of test arrangements

Critical Distinction: Flame Standard vs Product Flammability Test .58

IEC 60695-11-3 primarily defines the: **500 W standardized flame source**
and its: **confirmation method.**

ماده. It does not establish one universal pass/fail requirement for every product or
A product-specific or ماده-specific standard must define parameters such as:

- نمونه آزمون ;dimensions
- نمونه آزمون ;conditioning
- ;orientation
- ;exact flame application location
- ;burner angle
- ;application time
- ;number of flame applications
- ;afterflame time
- ;afterglow time
- ;dripping behaviour
- ;ignition of surrounding ماده;

- ;damage criteria
- ;classification
- final pass/fail criteria.

Therefore: **IEC 60695-11-3 apparatus conformity $\neq$ automatic product conformity.**

The standardized flame is the controlled ignition source used by another applicable test method.

59. Essential Pre-Test Verification Checklist

:Before using the apparatus for an actual fire-hazard test, verify

Common الزامات

- ✓ Correct IEC 60695-11-3 burner method selected
- ✓ Burner geometry compliant
- ✓ Burner clean and undamaged
- ✓ Correct fuel selected
- ✓ Fuel purity $\geq 98\%$
- ✓ Flow اندازه گیری $\pm 2\%$ tolerance
- ✓ Leak-free connections

- ✓ Correct flame-height gauge
- ✓ Inner blue cone approximately 40 mm
- ✓ Overall flame approximately 125 mm
- ✓ Stable and symmetrical flame
- ✓ Correct copper block
- ✓ Copper block 10.00 ± 0.05 g before drilling
- ✓ Copper block $\varnothing 9$ mm
- ✓ Correct 0.5 mm thermocouple
- ✓ Thermocouple IEC 60584-2 Class 1
- ✓ Thermocouple fully inserted
- ✓ Correct system اندازه گیری time/دما
- ✓ Timing tolerance ± 0.5 s
- ✓ Chamber volume ≥ 0.75 m³
- ✓ Draught-free environment
- ✓ Chamber background light ≤ 20 lx
- ✓ Extraction OFF during آزمون
- ✓ Burner stabilized ≥ 5 min
- ✓ Confirmation result 54 ± 2 s
- ✓ Three successive compliant determinations
- ✓ Copper block cooled naturally below 50 °C between runs

Additional Method A Checks

- Methane 965 ± 30 ml/min ✓
- 5 mm H₂O ± 125 فشار ✓ Back
- ✓ Adjustable air inlet correctly set
 - ✓ Air-inlet lock nut secured
- ✓ Inner blue cone 40 ± 2 mm during confirmation

Additional Method C Checks

- Correct methane or propane gas jet installed ✓
 - ✓ Correct fuel flow selected
 - ✓ Correct air flow selected
- ✓ Air supply essentially free from oil and water
- ✓ Separate gas and air circuits correctly connected
 - ✓ Correct flowmeters for both circuits

Engineering Significance of the Confirmation Test .60

One of the most important concepts behind IEC 60695-11-3 is that: **flame geometry alone does not prove thermal equivalence.**

:Two flames can both have

- ;a 40 mm inner blue cone
- ;a 125 mm overall height

while still transferring different amounts of heat.

:Possible causes include

- ;incorrect fuel flow
- ;inaccurate air flow
- ;incorrect burner geometry
- ;injector variation
- ;incorrect gas jet
- ;gas composition
- ;fuel فشار
- ;air فشار
- ;contamination

- burner دما;
- environmental airflow;
- اندازه گیری errors.

For this reason, the standardized flame is ultimately verified by its effect on a precisely defined thermal reference.

.That reference is the **10 g copper block**

A compliant flame must repeatedly heat that block from: **100 °C to 700 °C**

.in approximately: **54 seconds**

.61 The Complete IEC 60695-11-3 Control Philosophy

:The engineering logic of the standard can be summarized as

Control the burner geometry



Control the fuel quality



Control the fuel flow



Control the air supply / burner air inlet



Control the فشار conditions



Establish the specified flame geometry



Allow the burner to reach thermal equilibrium



Verify the 40 mm inner blue cone



Verify the approximately 125 mm overall flame



Measure thermal performance using the standardized copper block



Obtain 54 ± 2 s



Repeat until three successive results comply



Use the confirmed flame for the applicable fire-hazard test

This is why a properly designed 500 W flame-test apparatus is more than simply a burner and a gas-flow controller. It is a complete **controlled thermal test system**.



500W Flame Tester According IEC 60695-11-3

- Digital timer
 - Rotameter type flow controller
 - Gas فشار indicator
 - Automatic flame application on نمونه piece
 - Chamber size according to the standard
 - نمونه 2 axes linear mechanism positioning
 - Copper block and اندازه گیری (Not included in standard delivery)
- unit with WINDOWS software for verification of flame is as option

- **Nominal flame power:** 500 W
- **Flame type:** Premixed
- **Overall flame height:** ≈ 125 mm
- **Inner blue cone:** ≈ 40 mm
- **Copper block diameter:** $\varnothing 9 \pm 0.01$ mm
- **Copper block mass:** 10.00 ± 0.05 g before drilling
- **Thermocouple hole:** $\varnothing 0.5$ mm
- **Thermocouple:** 0.5 mm, Class 1
- **interval:** 100 ± 2 °C $\rightarrow$ 700 ± 3 °C
- **Required heating time:** 54 ± 2 s
- **Acceptable heating interval:** 52–56 s
- **Required confirmation:** 3 successive compliant tests
- **Cooling between runs:** naturally to ≤ 50 °C
- **Burner stabilization:** ≥ 5 min
- **Minimum chamber volume:** 0.75 m³
- **Background illumination:** ≤ 20 lx
- **Recommended equipment distance:** ≈ 55 mm

Method A

- **Fuel:** Methane (to be supplied by customer)
- **% Purity:** ≥ 98
- **Fuel flow:** 965 ± 30 ml/min

- **Back فشار:** $5 \text{ mm H}_2\text{O} \pm 125$
- **Flowmeter tolerance:** $\pm 2\%$
- **Manometer range:** $0-7.5 \text{ kPa}$
- **Burner tube ID:** $9.5 \pm 0.3 \text{ mm}$
- **Burner tube length:** $100 \pm 10 \text{ mm}$
- **Gas orifice:** $\text{Ø}0.9 \pm 0.03 \text{ mm}$
- **Minimum air-inlet area:** 225 mm^2

Method C - Methane

- **Fuel:** Methane (to be supplied by customer)
- **% Purity:** ≥ 98
- **Fuel flow:** $965 \pm 30 \text{ ml/min}$
- **Air flow:** $6.3 \pm 0.1 \text{ l/min}$
- **Expected fuel back فشار:** $170 \text{ mm H}_2\text{O}-110$
- **Expected air back فشار:** $40 \text{ mm H}_2\text{O}-20$
- **Gas jet:** $\text{Ø}0.7 \text{ mm}$

Method C - Propane

- **Fuel:** Propane (to be supplied by customer)
- **% Purity:** ≥ 98
- **Fuel flow:** $380 \pm 15 \text{ ml/min}$

Air flow: 5.9 ± 0.1 l/min •
Expected fuel back فشار: 205 mm H₂O-135 •
Expected air back فشار: 35 mm H₂O-15 •
Gas jet: Ø0.5 mm •